

## **Original Research Article**

### **QUALITATIVE ASSESSMENT OF X-RAY MACHINES' MECHANICAL PARAMETERS AT SOME SELECTED DIAGNOSTIC CENTRES IN NIGERIA**

#### **ABSTRACT**

**Introduction:** X-ray machines' mechanical parameters are potential influencers of image quality and radiation exposure of patients hence, the need to assure their good performance prior clinical services. The scope of quality control (QC) measurements performed on diagnostic x-ray machines in Nigeria varied from centre to centre due to lack of the required QC equipment. This study assessed the present status of x-rays machines used for common diagnostic x-ray examinations in Nigeria.

**Materials & Methods:** Total of 112 x-ray machines from 106 diagnostic centres from six geopolitical zones in Nigeria were considered. Structured questionnaires and Diavolt Dosimeter were respectively used for data collection and measurement of parameters, namely Half-Value Layer (HVL), tube voltage (kVp) reproducibility, kVp accuracy and beam output linearity/stability.

**Results:** By zonal distribution of x-ray units, the highest number (36%) and the least (7%) was from the south-west and south-south respectively. In all, 71% were owned by private institutions, 71% were non-mobile, 64% were operated on 3-phase generator and 35% were within the age of ten years. The HVLs of 97% of the x-ray units were within the standard thickness of 2.3 mmAl (at 80 kVp, 100 cm FFD), 88% have acceptable kVp reproducibility and 51% have kVp accuracy within  $\pm 5\%$ . Only x-ray units (64%) operated on 3-phase generator produced beam output that are within acceptable stability.

**Conclusion:** This study showed that many diagnostic centres, especially those in the south-south region, are yet to register with the regulatory authority, some (65%) of the x-ray units are aged (>10 years) and about 49% of the units failed kVp accuracy test.

**Keywords:** Diagnostic radiology, Quality Assurance, Quality Control, image quality, x-ray unit, mechanical parameters, radiation exposure

## **INTRODUCTION**

Since the discovery of x-ray in 1895 by Wilhelm Rontgen, medical imaging with x-rays has become an indispensable healthcare delivery procedure in the diagnosis and treatment of diseases [1]. The major concern of clinicians in medical x-ray imaging is how to obtain image quality that is consistent with clinical diagnosis of the disease at a minimum radiation dose to patients [2, 3]. This is because; the medical use of ionizing radiation has the potential of significantly increasing the exposure of the population to ionizing radiation if the principles of radiation protection are compromised. Hence, the need for proper quality assurance procedures in diagnostic radiology to reduce to the barest minimum, the detrimental health effect of over exposure to ionizing radiation on patients, operators and the general public.

The World Health Organization (WHO) defines quality assurance (QA) programme in diagnostic radiology as an organized effort by the staff operating the radiation facility to ensure that the diagnostic images produced are of sufficiently high quality so that they consistently provide adequate diagnostic information at the lowest possible cost and with the least possible exposure of the patient [4].

The roles of quality assurance program in diagnostic radiology cannot be overemphasized as it helps the x-ray facility to consistently producing optimal radiological information with minimal radiation dose, as low as reasonably achievable. An integral part of quality assurance program is the quality control measurements of mechanical parameters of x-ray units, especially those that have direct bearing on the magnitude of ionizing radiation emitted from the x-ray tube. Some of these mechanical parameters are beam alignment, beam collimation, kVp reproducibility, kVp

accuracy, time accuracy, half value layer (HVL), leakage test, linearity test, machine output, among others [5].

Most diagnostic centres in Nigeria lack the required quality control equipment and personnel, for testing the performance characteristics of their machines' mechanical parameters and this has prevented their x-ray machines from undergoing comprehensive quality control measurements.

Therefore, this study was carried out to assess the present performance characteristics of some of the mechanical parameters of x-ray units at some selected diagnostic centres in Nigeria and give recommendations, based on findings, that would improve the quality of diagnostic images produced at optimal radiation dose to patients.

## **MATERIALS AND METHODS**

### *Selection of Diagnostic Centres*

The records of diagnostic centres, who registered with the Nigerian Nuclear Regulatory Authority (NNRA), Abuja and were captured under the Regulatory Authority Information System (RAIS) as at the year 2016 were assessed. The diagnostic centres with complete records of their exact locations and relevant information about their x-ray machines were extracted from RAIS for this study.

Out of about 800 diagnostic centres extracted from RAIS, only 106 (13%) centres satisfied the inclusion criteria for this study. The Management of these centres were thereafter contacted and their consents were sought for a visit to their facility. The centres were also categorized into the six geo-political zones in Nigeria, namely: North Central, North West, North East, South South, South West and South East. The centres were also classified based on the ownership of the facility namely: Federal Government (Teaching hospital), State Government and Private owned centres. There are total of 112 x-ray machines in all the 106 diagnostic centres considered in this study and their mechanical parameters, whose performance characteristics were measured are Half Value Layer (HVL), kVp reproducibility, kVp accuracy and machine output consistency. The parameters tested are limited by the capability of the dosimeter used for measurement.

In addition, relevant questionnaires were designed and distributed to the Radiographers/Operators in charge of the diagnostic facilities to obtain machine data such as year of manufacture, model name/number, type of generator, total filtration, etc. Other information obtained from the centres was the daily patient workload.

Evidence of ethical approval was presented at the diagnostic centres before access was granted into their facilities for various measurements on the x-ray machines.

### ***Calibration of Diavolt Dosimeter***

The dosimeter used for measurement of x-ray machines' mechanical parameters in all the diagnostic centres is a multipurpose Diavolt dosimeter, model 330 and was manufactured by the Gammex PTW, USA. Prior to its use at the various diagnostic centres, it was subjected to calibration at the national Secondary Standard Dosimetry Laboratory (SSDL), University of Ibadan, Ibadan in Oyo State. This SSDL is located in the radiation dosimetry and training institute of the NNRA, Abuja.

The calibration of the Diavolt dosimeter was performed against the reference ionization chamber, Exradin A3, using the diagnostic x-ray beam energy source at SSDL. The Ionization chamber and Diavolt dosimeter were exposed in succession to the same x-ray energy source, which was set at a constant tube voltage (kVp) of 80 and varying tube loading (12.5 – 75.0) (mAs). The distance of the detectors (Ionization chamber or Diavolt) from the x-ray source was kept at 100 cm. The detectors were exposed three times each using the same machine settings and the mean and standard deviation were calculated and recorded. The detectors were carefully hanged to ensure that backscatter influence was avoided [5].

### ***Measurement Set-Up at Each Diagnostic Centre***

At each diagnostic centre, the calibrated Diavolt dosimeter was mounted (shown in fig. 1) on an Aluminium retort stand, which has a movable clamp so that the position of the dosimeter can be easily adjusted in relation to the central axis of the x-ray beam and the patient's couch (6). The detector-to-table distance (DTD) was kept at 25cm to prevent the influence of scatter on the table and the aluminum stand. The values of the x-ray tube loading (mAs) and tube voltage (kVp) for each measurement were set on the control console with the assistance of the operator at each of the centre. The ranges of values covered for each measured quantity were guided by the operational data entry in the questionnaire previously completed by the centre.

### ***Half Value Layer Measurements***

This was done by keeping the focus-detector distance (FDD) setting at 100 cm while the tube voltage and tube loading were set at 80 kVp and 20 mAs respectively. Dosimeter readings were first taken with inherent filter only (that is, no filter was placed between the x-ray source and the dosimeter) and thereafter, an Aluminum filter is added in steps of 1mm thickness until the added filtration was 5 to 6 mm thickness, depending on the initial value taken with only inherent filter. The readings were recorded and tabulated.

### ***kVp Reproducibility and Accuracy Measurements***

While maintaining the same focus-detector distance setting of 100 cm, the kVp reproducibility was checked by taking three different exposures without changing the kVp and mAs settings and the values of kVp displayed on the dosimeter were recorded. This was to verify whether kVp set by the radiographer were the same from exposure to exposure. The coefficient of variation (CV) in equation 1 was used to determine the kVp reproducibility. The CV should be  $< 0.2$  for good kVp reproducibility.

$$CV = \frac{SD}{M} \times 100\% \quad (1)$$

where SD is the Standard deviation and M is the mean of the values

The kVp accuracy was also checked by taking exposures with varying settings of kVp and constant mAs and recorded the deviation between the kVp set on the control console against the kVp measured by the dosimeter. The accuracy should be within  $\pm 5\%$ . All readings were recorded and mean values were tabulated.

$$\text{kVp accuracy} = \frac{\text{kVp}_{\text{set}} - \text{kVp}_{\text{measured}}}{\text{kVp}_{\text{set}}} \times 100\% \quad (2)$$

### ***Machine Output Consistency Measurements (Linearity Test)***


While the settings of Diavolt dosimeter and the tube voltage was kept at a fixed FDD of 100 cm and 80 kVp respectively, the tube loading (mAs) was varied from 20 to 80 mAs in steps of 10 mAs. The tube loading was set to cover the range of mAs commonly used for patient's exposure at each diagnostic centre. The beam output (mGy/mAs) was recorded and tabulated. The maximum and minimum beam output was observed and equation 3 was used to calculate the

machine output consistency. The value should be less than 0.1 for good machine output consistency.

Machine output consistency was further checked by maintaining the settings of Diavolt dosimeter and the tube loading at a fixed FDD of 100 cm and 20 mAs respectively, the tube voltage was varied from 40 kV to 80 kV in steps of 10 kV. The tube voltage was set to cover the range of kVp commonly used for patient's exposure at each diagnostic centre. The graph of tube output was plotted against kVp for each centre and the linearity was assessed using the formula below.

$$\text{Linearity} = \frac{X_{\max} - X_{\min}}{X_{\max} + X_{\min}} \quad (3)$$

where X is the beam output in mGy/mAs.

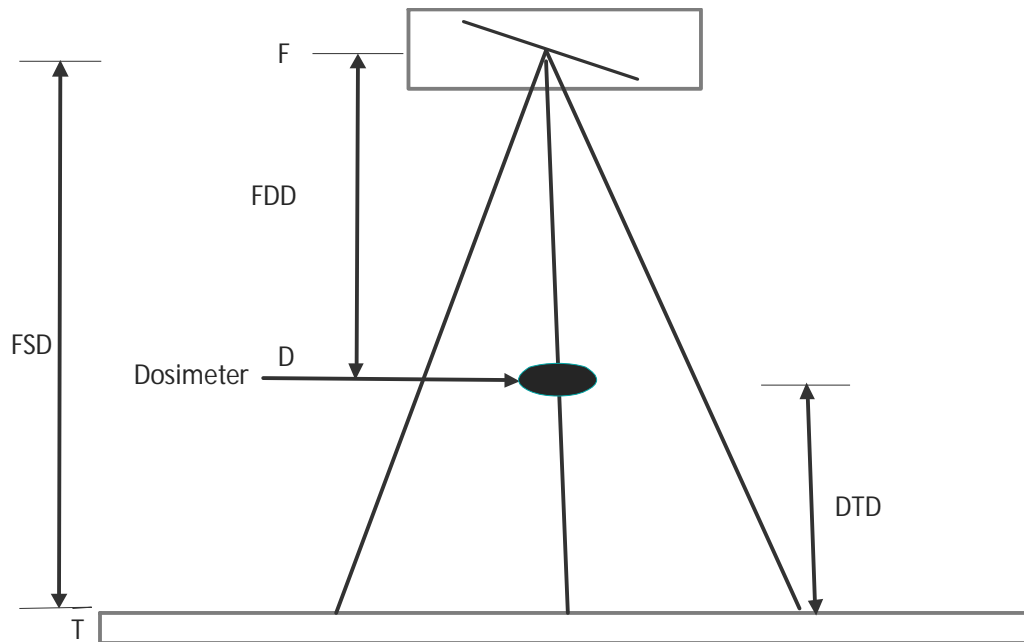

**Fig. 1: Experimental Setup for all Measurements at Each Centre.**

*FSD = Focus-to-Skin Distance, FDD = Focus-to-Detector Distance, DTD = Detector-to-Table Distance, T = Table, F = X-ray Tube Focus, D = Detector*

## **RESULTS AND DISCUSSION**

### *Analysis of Data from Diagnostic Centres*

A total number of 112 diagnostic x-ray machines were assessed from 106 diagnostic centres considered for this study. The classification of the diagnostic centres based on the ownership and the geo-political zone to which each belongs are presented in Table 1. Information on x-ray machine with respect to their location (mobile or fixed) and generator types (single or 3-phase frequency) are presented in Table 2 (a) while the age of the various x-ray machines was grouped and presented in Table 2 (b). The daily patient's workload on x-ray machine at each centre is presented in Table 3.

The distribution of x-ray units considered in this study showed that the majority (36%) of the x-ray units were in the south western zone, most (71%) were owned by private institutions, 71% were fixed units and 63% were operated on 3-phase generator.

With respect to the age of the x-ray machines, it was observed that, the year of manufacture of about 41% of the x-ray machines were not available because they had faded away from the machines and could not be clearly seen. Of the remaining x-ray machines, 31% were less than ten years of age, 17% were within ten to twenty years and twelve (12%) were above 20 years of age from the year of data acquisition.

### ***Response of Diavolt Dosimeter against Ionization Chamber***

The response, which is the degree of reliability, of Diavolt dosimeter (Field detector) to a known value of beam quality as against the response of the ionization chamber (Reference detector) operated under the same condition is presented in Table 4. The variation between the two detectors was found to range from 0.77 to 1.32.

### ***Half Value Layer (HVL) of X-ray Machines***

The Half Value Layer (HVL) measurement was carried out at each centre in order to determine the total filtration (inherent and added) in the x-ray tube assembly, thereby assessing the extent to which low energy x-rays beam have been removed before reaching the patient during medical imaging at each centre. The analysis of the measured HVL of 112 diagnostic x-ray machines at the six geopolitical zones showed that the HVL of the majority (97%) of the x-ray machines were within the standard thickness of 2.3 mm Al at tube voltage of 80 kVp and focus to detector distance (FDD) of 100 cm [6]. The remaining x-ray machines (3%) have HVL that is less than 2.3 mm Al as seen in Table 5.

### ***kVp Reproducibility***

The coefficient of variation between three different exposures of kVp at various diagnostic centres showed good reproducibility i.e. coefficient of variation  $< 0.2$  (7,8) for 91% of the x-ray units in the North central, 82% in the North East, 100% in the North West, 88% in the South-South, 88% in the South West and 80% in the South East. This implies that majority of the x-ray machines in all the geopolitical zones had good kVp reproducibility as seen in Table 6. However, some centres had bad kVp reproducibility, which may be due to the age of the x-ray machines.

### ***kVp Accuracy***

The kVp accuracy for 112 X-ray machines in the six geo-political zones was calculated and analyzed as presented in Table 7. Although, it is expected that the deviation between the kVp set by the operator and the kVp measured by detector is within  $\pm 5\%$  [4]. However, it was observed that only 12 (36%) centres in the North Central zone, 6 (54%) in the North East, 7 (70%) in the North West, 5 (40%) in the SouthSouth, 18 (45%) in the South West and 3(30%) in the South

East zones were within the  $\pm 5\%$  limit. This means that only 45% of all the diagnostic units considered in this study produced kVp that is accurate within  $\pm 5\%$ .

### ***Tube Output Linearity***

Tube output linearity test carried out on 112 diagnostic x-ray machines in six geopolitical zones showed varied level of consistency and stability with respect to the applied power source/generator and is presented in Table 8. It was observed that the x-ray units operated on single phase generator produced x-ray beam output that is characterized by inconsistency due to power interruption/ fluctuation. Some of the x-ray units in this category were found in the state and private institutions. Whereas, most of the x-ray machines at the Federal/teaching institutions were operated on 3-phase generator, which helped in stabilizing their x-ray beam output. As seen in Table 8, only 64% of the x-ray units considered in this study produced stable beam output.

**Table 1:** Distribution of Diagnostic Centres based on Ownership and Geographical Location

| <b>Geo-political zone</b> | <b>Private</b> | <b>State Government</b> | <b>Federal Government</b> | <b>Total</b> |
|---------------------------|----------------|-------------------------|---------------------------|--------------|
| North Central             | 24             | 2                       | 7                         | 33           |
| North West                | 8              | -                       | 2                         | 10           |
| North East                | 3              | 3                       | 5                         | 11           |
| South South               | 7              | -                       | 1                         | 8            |
| South West                | 30             | 5                       | 5                         | 40           |
| South East                | 8              | -                       | 2                         | 10           |
| Total                     | 80             | 8                       | 22                        | 112          |

**Table 2 (a):** Information on Diagnostic X-ray Machines at Various Diagnostic Centres

| <b>Geo-political zone</b> | <b>No of Mobile X-ray Unit</b> | <b>No of Fixed X-ray Unit</b> | <b>No with Single phase Generator</b> | <b>No with 3-phase Generator</b> |
|---------------------------|--------------------------------|-------------------------------|---------------------------------------|----------------------------------|
|---------------------------|--------------------------------|-------------------------------|---------------------------------------|----------------------------------|

|               |    |    |    |    |
|---------------|----|----|----|----|
| North Central | 11 | 22 | 17 | 16 |
| North West    | 5  | 6  | 7  | 4  |
| North East    | 3  | 7  | 2  | 8  |
| South South   | 1  | 7  | 1  | 7  |
| South West    | 12 | 28 | 14 | 26 |
| South East    | 1  | 9  | 1  | 9  |
| Total         | 33 | 79 | 42 | 70 |

**Table 2 (b):** Age of X-ray Machines at Various Diagnostic Centres

| Geo-political zone | ≤ 5 years | > 5 ≤ 10 years | > 10 ≤ 15 years | > 15 ≤ 20 years | > 20years | *NA |
|--------------------|-----------|----------------|-----------------|-----------------|-----------|-----|
| North Central      | 6         | 5              | 2               | 3               | 6         | 11  |
| North West         | 3         | NA             | 2               | NA              | 1         | 5   |
| North East         | NA        | 1              | 4               | 1               | 2         | 2   |
| South South        | NA        | 3              | 1               | 1               | NA        | 3   |
| South West         | 6         | 7              | 1               | 3               | 3         | 20  |
| South East         | 2         | 2              | 1               | NA              | NA        | 5   |
| Total              | 17        | 18             | 11              | 8               | 12        | 46  |

\*NA – Not Available

**Table 3:** Daily Patient's Workload on X-ray machine at Various Diagnostic Centres

| Geo-political zone | < 10 Patients | > 10 < 20 Patients | > 20 < 30 Patients | > 30 patients |
|--------------------|---------------|--------------------|--------------------|---------------|
|                    |               |                    |                    |               |

|               |    |    |    |    |
|---------------|----|----|----|----|
| North Central | 2  | 17 | 4  | 10 |
| North West    | 1  | 5  | 1  | 4  |
| North East    | 2  | 3  | 2  | 3  |
| South South   | 1  | 2  | 2  | 3  |
| South West    | 5  | 16 | 9  | 10 |
| South East    | 2  | 3  | 3  | 2  |
| Total         | 13 | 46 | 21 | 32 |

**Table 4:** Response of Diavolt Detector and Ion Chamber during Calibration at SSDL

| Tube Loading<br>(mAs) | Air Kerma ( $\mu\text{Gy}$ ) |             |             |
|-----------------------|------------------------------|-------------|-------------|
|                       | Diavolt                      | Ion Chamber | % Variation |
| 12.5                  | 731.9 $\pm$ 1.6              | 723.5       | 1.16        |
| 25.0                  | 1460.0 $\pm$ 1.8             | 1441.0      | 1.32        |
| 50.0                  | 2905.0 $\pm$ 1.9             | 2881.0      | 0.83        |
| 75.0                  | 4345.0 $\pm$ 2.0             | 4312.0      | 0.77        |

**Table 5:** Analysis of HVL (80 kVp & 100cm FDD) at Various Diagnostic Centres

| Geo-political Zone | Number of X-ray machine<br>with filter < 2.3 mm Al | Number of X-ray machine with<br>filter $\geq$ 2.3 mm Al |
|--------------------|--|---|
| North Central      | 1  | 32  |
| North West         | 1  | 10  |
| North East         | Nil  | 10  |

|             |     |     |
|-------------|-----|-----|
| South South | Nil | 8   |
| South West  | 1   | 39  |
| South East  | Nil | 10  |
| Total       | 3   | 109 |

**Table 6:** kVp Reproducibility at Various Diagnostic Centres

| <b>Geo-political Zone</b> | <b><math>\leq 2\%</math><br/>(Good<br/>Reproducibility)</b> | <b>X-ray machine<br/>with good<br/>reproducibility<br/>(%)</b> | <b><math>&gt; 2\%</math><br/>(Bad<br/>Reproducibility)</b> |
|---------------------------|---|--|--|
| North Central             | 30  | 91   | 3  |
| North West                | 9   | 82   | 2  |
| North East                | 10  | 100  | *NA  |
| South South               | 7   | 88   | 1  |
| South West                | 35  | 88   | 5  |
| South East                | 8   | 80   | 2  |
| Total                     | 99  | 88   | 13   |

\*NA – Not Available

**Table 7:** kVp Accuracy at Various Diagnostic Centres

| <b>Geo-political</b> | <b>Machine setting</b> | <b>Machine setting</b> | <b>Machine setting</b> |
|----------------------|------------------------|------------------------|------------------------|
|----------------------|------------------------|------------------------|------------------------|

| <b>Zone</b>   | <b>within <math>\pm 5\%</math></b> | <b>within <math>\pm 10\%</math></b> | <b><math>&gt; \pm 10\%</math></b> |
|---------------|------------------------------------|-------------------------------------|-----------------------------------|
| North Central | 12                                 | 11                                  | 10                                |
| North West    | 6                                  | 4                                   | 1                                 |
| North East    | 7                                  | 1                                   | 2                                 |
| South South   | 5                                  | 2                                   | 1                                 |
| South West    | 18                                 | 15                                  | 7                                 |
| South East    | 3                                  | 2                                   | 5                                 |
| Total         | 51                                 | 35                                  | 26                                |

**Table 8:** X-ray Beam Linearity at Various Diagnostic Centres

| <b>Geopolitical Zone</b><br><b>(No of x-ray Unit)</b> | <b><math>\leq 0.1</math> (stable)</b> | <b><math>&gt; 0.1</math> (unstable)</b> |
|---|---------------------------------------|---|
| North Central (33)                                    | 21 (64%)                              | 12 (36%)                                |
| North West (11)                                       | 5 (45%)                               | 6 (55%)                                 |
| North East (10)                                       | 8 (80%)                               | 2 (20%)                                 |
| South South (40)                                      | 20 (50%)                              | 20 (50%)                                |
| South West (8)  | 6 (75%)                               | 2 (25%)                                 |
| South East (10)                                       | 4 (40%)                               | 6 (60%)                                 |
| Total (112)   | 64 (57%)                              | 48 (43%)                                |

## CONCLUSION

X-ray machines mechanical parameters of some selected diagnostic centres were assessed using multipurpose Diavolt dosimeter. The result showed that almost half of the x-ray centres lack machine maintenance culture. This may affect the quality image produced by the x-ray system and the overall effect would be inconsistency in patients' radiation exposure and absorbed dose. Further study is aim at quantify the absorbed dose received by patients at these centres.

## REFERENCES

1. John Pearn 2015. The Discovery of X-rays: Challenges to Societal Beliefs and Professional Paradigms. Australian and New Zealand Society of the History of Medicine journal. Vol. 17; (1): 53-72.
2. Akinlade B. I., Farai, I. P. and Okunade A. A. 2012. Survey of dose area product received by patients undergoing common radiological examinations in four centres in Nigeria. *Journal of Applied Clinical and Medical Physics* 13 (4):1-9.
3. Jibiri N. N. and Olowookere C. J. 2016. Patient dose audit of the most frequent radiographic examinations and the proposed local diagnostic reference levels in southwestern Nigeria: Imperative for dose optimization. *Journal of Radiation Research and Applied Sciences*. Vol. 9, 247 – 281.
4. Kareem A. A., Hulugalle S. N., Al-Hamadani H. K. A Quality Control Test for General X-Ray Machine. *World Scientific News* 90 (2017) 11-30.
5. Dance D.R, Christofides S., Maidment A.D.A, McLean I.D and Ng K.H 2014. Diagnostic radiology physics: A handbook for teachers and Students. IAEA Vienna.
6. National Council on Radiation Protection and Measurements (NCRP) 1989. Medical X-ray, electron beam, and gamma ray protection for energies up to 50 MeV (equipment design, performance and use). NCRP report no.102. Bethesda, Md:
7. International Atomic Energy Agency (IAEA). 2007. Dosimetry in diagnostic radiology, International Code of Practice, IAEA technical report series 457, Vienna.

8. Boone J, Dianna D, Cody M., Jane R. Donald F and Frey G. 2002. Quality control in diagnostic Radiology. AAPM report no. 74
9. Jeff Shepard M. S., Pei-Jan Paul Lin C, John Boone C.-C. M., Dianna D. 2002. Quality Control in Diagnostic Radiology. Report of Task Group Diagnostic X-ray Imaging Committee, College Park, AAPM Report No. 74. Medical Physics Publishing. 0271-7344.