

## Original Research Article

### **Design and construction of a system for measuring carbon monoxide, hydrogen and methane concentrations in a co-current downdraft biomass gasifier**

#### **Abstract**

Gasification is the process of producing combustible gases from solid materials such as coal, biomass or solid waste. Our laboratory of Space Physics and Energy has two experimental gasifiers producing synthetic gases whose natures and concentrations must be determined. To do this, lower-cost sensors were purchased and used for determining the concentration of carbon monoxide, hydrogen and methane in synthetic gas produced by a wood fired co-current downdraft gasifier. These sensors have a chemical sensing element based on a layer of tin dioxide (SnO<sub>2</sub>); whose resistivity is sensitive to nature of the gas between two sensing electrodes. This property gives these sensors a resistive electrical model whose measurand is the concentration of the input gas. This study is therefore the physical and mathematical modeling of these synthesis gas concentration sensors  $[c] = g(R)$  in order to allow their electronic exploitation with a microcontroller.

**Keywords:** Gasification, Modelling, Concentration, Carbon monoxide, Hydrogen, Methane

#### **1. Introduction**

Burkina Faso, efforts to reduce energy dependence (of populations and industries on fossil resources and wood) are being carried out through the development of renewable energy sources such as photovoltaic and thermal solar [1], [2]. To make our contribution to this concern, the Laboratory has therefore embarked on the construction of experimental gasifiers producing synthetic gases usable for the production of electricity. From May to August 2022, a first downdraft gasifier was designed and successfully tested two wood fired downdraft biomass in Burkina Faso [3], [4]. A second gasifier was designed and built from September to December 2022 in order to overcome design flaw that was

found in the first gasifier during the testing's. The two gasifiers built are of the co-current type which are already used in industry from 100kW and above for their suitability, as well as their relative ease of manufacturing in developing countries. As a reminder, gasification is the process of producing combustible gases from solid materials such as coal, biomass or solid waste. However, faced with the diversity of combustion materials, one of the problems is to detect the nature of the gases produced as well as their concentrations with precision. The laboratory already has analyzers such as Testo 310, Bacharach (Fyrite Pro, Fyrite Intech 120, Monoxor III) with a measuring range of 1000 to 2000 ppm of carbon monoxide and which

**Commented [U1]:** Design and construction of a co-current downdraft biomass gasifier for measuring carbon monoxide, hydrogen and methane concentrations: A suggestion

**Commented [U2]:** The content of the abstract should include background of the study, brief statement of the problem, brief method followed, results and brief conclusion. In addition, concentration of H<sub>2</sub>, CO and CH<sub>4</sub>. suppose to be captured in the Abstract

**Commented [U3]:** Personal pronoun such as we, our should be avoided throughout the text.

**Commented [U4]:** The entire areas in blue should be rephrase, emphasis should be given to introducing previous related works carried out by the other researchers not like trying to discuss your own results and peculiarities...

saturate very quickly for higher concentrations.

Unfortunately, flue gas analyzers we have on hands are not built for continuous operation.

Because we out passed that manufacturer's restriction using the analyzers for 30 minutes or hours, we ended up damaging Oxygen and Carbon monoxide sensors. Replacing these sensors appeared out of reach for Bacharach® analyzers, because these sensors are relatively costly for underdeveloped countries as Burkina Faso and not suited for long run usage (maximum 5 minutes recommended by the manufacturers). Testo @ 310 XL analyzer doesn't didn't give leave us the possibility of replacing sensors. That analyzer should be sent back to a specialized manufacturer's maintenance center endowed with special tools for opening that hand held gas analyzer, replacing the bad sensors and recalibrating these. Therefore, we had no choice than looking for other solutions.

As said by Yulin Kong et al. [5]: "SnO<sub>2</sub> has been extensively used in the detection of various gases. As a gas sensing material, SnO<sub>2</sub> has excellent physical-chemical properties, high reliability, and short adsorption-desorption time". We also found in the literature that other authors were already using cheap gas monitoring sensors for industrial applications [6], [7], [8]. We also found that a microcontroller can be used to acquire data from numerous sensors, compute several mathematical functions and display these values [9], [10], [11]. This is why we anticipated that the combination of these gas sensors with a microcontroller would constitute a cost-effective replacement solution for monitoring gas concentrations in our biomass gasifiers and decided to build an experimental prototype system for measuring these gases, in particular carbon monoxide, hydrogen and methane.

## 2. Materials and methods

### 2.1 Experimental setup

The gasifier used in this work is composed of several functional units:

- The reactor
- The cyclone
- The condenser
- The filter

Figure 1 bellow shows the overview of these different parts. MQ gas sensors are located on a sampling box that draw small amount of synthetic gas cleaned of tar and water vapor by the cyclone separator, the condenser and the filter.

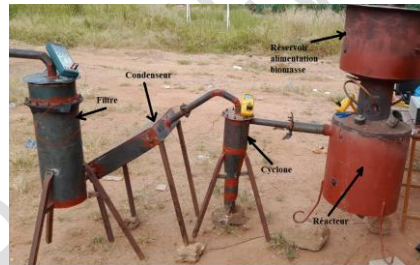


Figure 1 : Experimental setup

### 2.2 Methods

The main gases whose concentrations we want to detect and measure are: H<sub>2</sub>, CO and CH<sub>4</sub>. the respective sensors are: MQ-8, MQ-7, MQ-4.

**Commented [U5]:** Please recheck this line for clarity ; this don't suppose to be here in introduction.....

**Commented [U6]:** The entire areas in reds should be rephrase, emphasis should be given to introducing previous related works carried out by the other researchers....

**Commented [U7]:** Replace « we » with it w as .....

**Commented [U8]:** Avoid using «We» (personal pronoun). You can start with It was

**Commented [U9]:** It was

**Commented [U10]:** Please remove it

### 2.2.1 Chemical behaviour of MQ gas sensors

The basic chemical element of MQ gas sensors is a tin dioxide ( $\text{SnO}_2$ ) layer. From an electrical point of view, a perfect  $\text{SnO}_2$  crystal exhibits insulating behavior, due to its wide bandgap. Depending on the purity of the material, we note in the literature a large dispersion of the experimental values of the bandgap which varies between 2.25 to 4.3 eV [12]. On the basis of the results obtained by Jacquemin [13], we can consider that the band gap is direct and that the value of this band gap at room temperature varies between 3.5 to 4 eV. At the opposite, the real crystal has a semiconductor character. This behavior results from deviations from stoichiometry and is closely linked to the presence of oxygen vacancies leading to the presence of donor-type energy levels inside the bandgap [14].

### 2.2.2 Operating principle

The electrical properties of tin oxide layers are influenced by the gaseous chemical environment in contact with the layer. Thus, the absorption by physisorption or chemisorption of chemical species on the surface of the layer modifies its conductivity by a modification of the electronic states of the semiconductor by movement of electrons from the valence band towards the conduction band. This process is done in three steps [12]. Firstly, the layer is brought into contact with air and the adsorption of dioxygen molecules causes their dissociation and ionization in  $\text{O}^-$  form (the most stable species at high temperature) by tearing off an electron from the band. conduction of the layer. Secondly, the reducing gas molecules, to be detected, react on the surface with the anions releasing an electron towards the conduction layer of the oxide and varying its electrical conductivity depending on the number of active oxidation sites and the number of gas molecules chemisorbed on the surface. Thirdly, following the cessation of the introduction of the gas, the oxygen present in the atmosphere adsorbs again on the surface of the oxide, returning to the equilibrium state established during the first process. However, this return to the equilibrium state assumes the absence of phenomena of poisoning of the sites by secondary molecules resulting from oxidation reactions. [14]

Given the above, the resistivity of the tin oxide layer varies depending on the concentration of environmental gases. We can model it by a variable resistance depending on the concentrations as shown on Figure 2 below.




Figure 2 : Electrical model of a MQ gas sensor

Commented [U11]: Be using reported speech although

Commented [U12]: Replace with was and apply to all related places.

### 2.2.3 Presentation of the sensors

The following Figure 3 is the representation of a gas MQ sensors.

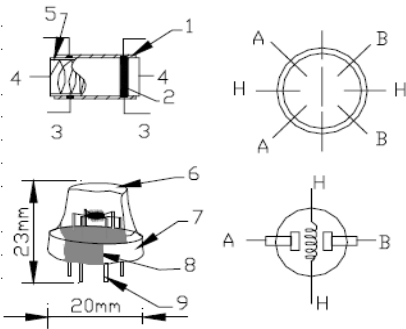


Figure 3 :MQ gas sensors structure

Each SnO<sub>2</sub> sensor is composed of the elements in Table 1 below:

Table 1 : Constitutes of a gas sensor

Parts	Materials
1 Gas sensing layer	SnO <sub>2</sub>
2 Electrode	Au
3 Electrode line	Pt
4 Heater coil	Ni-Cr alloy
5 Tubular ceramic	Al <sub>2</sub> O <sub>3</sub>
6 Anti-explosion network	Stainless steel gauze (SUS313 100-mesh)
7 Clamp ring	Bakelite
8 Tube pin	Copper plating Ni

### 2.3 Mathematical model of the sensors

Depending on the type of sensor, the manufacturer has provided a standard catalog of correlation curves that was used.

$$\text{Curves } \log\left(\frac{R_s}{R_0}\right) = f([C]_{(ppm)})$$

are plotted on a logarithmic scale and are linear. By changing variables

$$Y = \log\left(\frac{R_s}{R_0}\right) \text{ and } X = \log([C]_{(ppm)}),$$

these equation becomes:  $Y = A * X + B$ .

Using the coordinates of two points

$(X_1, Y_1)$  and  $(X_2, Y_2)$ ,

We get A and B :

$$A = \frac{Y_1 - Y_2}{X_1 - X_2} \text{ and } B = Y_2 - \left(\frac{Y_1 - Y_2}{X_1 - X_2}\right) * X_2$$

Subsequently, we will use the calibration curves provided in the technical datasheets to determine the coefficients A and B for each sensor according to the type of gas to be detected.

As said by "SnO<sub>2</sub> based MOS gas sensors are most popular for sensing a wide range of gases. Selection of a gas sensing material is crucial due to the fact that selectivity is an important characteristic for designing efficient gas sensing devices" [15]. We will therefore selected the appropriate sensor for each gas we are willing to sense in paragraphs below.

#### 2.3.1 Dihydrogen and derivatives

These gases were detected by the MQ8 sensor.

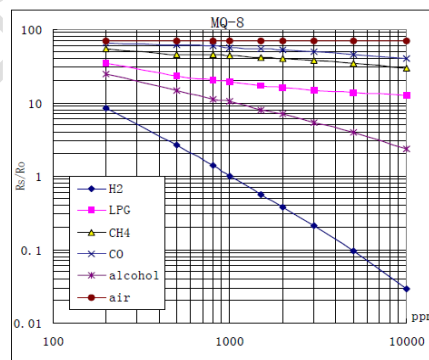


Figure 4 : MQ-8 sensitivity to different gases

As can be seen on Figure 4 above: the sensitivity of MQ-8 sensor varies depending on the gas it detects. Hydrogen has the highest variation slope, then come alcohol with a smaller slop variation. Liquefied Petroleum Gas, methane carbon monoxide has very small variation slopes, similar to that of the air. Therefore, we used MQ-8 for measuring hydrogen concentration in flue gas.

Commented [U13]: We used

Commented [U14]: Remove it

In Table 2 below, calculated the parameters A and B above for hydrogen presented.

Table 2 : Calculated values of A and B for MQ-8

AIR	70	100	0	1,845
	70	1000		
CO	Y=log (RS/RO)	X=log (ppm)	A	B
	50	3000	-0,18534	2,343
	40	10000		
CH4	Y=log (RS/RO)	X=log (ppm)	A	B
	40	2000	-0,17875	2,1921
	30	10000		
LPG	Y=log (RS/RO)		A	B
	20	800	-0,1570	1,7568
	15	5000		
ALCOL	Y=log (RS/RO)	X=log (ppm)	A	B
	4	5000	-0,61074	2,8612
	7	2000		
H2	Y=log (RS/RO)	X=log (ppm)	A	B
	1	1000		
	0,03	10000	-1,5229	4,5686
AIR				
$\log\left(\frac{R_s}{R_o}\right) = 1,8451 \Leftrightarrow \frac{R_s}{R_o} = 10^{(1,8451)} = 70$				
H2				
$\log\left(\frac{R_s}{R_o}\right) = -1,5228 * \log(x) + 4,5686$ $= A * \log(x) + B$				

### 2.3.2 Dihydrogen carbon monoxide and others

These gases were detected with MQ-7 sensor with sensitivity characteristics reported on Figure 5 below. It can be seen there that hydrogen has the highest slope variation followed by carbon monoxide. Furthermore, the two curves were almost parallels. Therefore, in the case of gasification where carbon monoxide and hydrogen are the main components, ways should be found to determine separate concentration of either hydrogen or

carbon monoxide and deduce concentration of the other.

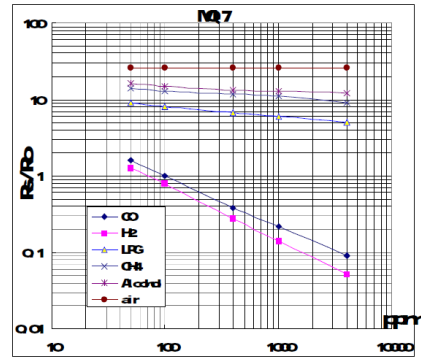


Figure 5 : MQ-7 sensitivity characteristics

Parameters A and B for MQ-7 are calculated in Table 3 : Parameters A and B calculation for MQ-7 below.

Only equation for CO is given on Table 3. H<sub>2</sub> was calculated from MQ-8 and deduced from MQ-7. For example, if MQ-8 reads a concentration [H<sub>2</sub>] of hydrogen and MQ-7 reads concentration [H<sub>2</sub> + CO], concentration [CO] as MQ-7 reading minus MQ-8 reading was then calculated.

### 2.3.3 Methane and derivatives.

These gases were detected with MQ-4 sensor. Sensitivity characteristics of MQ-4 sensor is given on Figure 6 below:

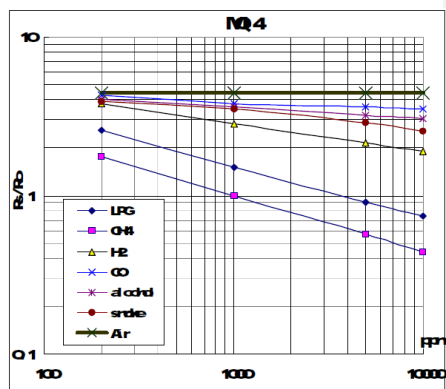


Figure 6 : Sensitivity characteristics of MQ-7

Table 3 : Parameters A and B calculation for MQ-7

Name of gas	Y=log (RS/R0)	X=log (ppm)	A	B
AIR	26	50	0	1,4150
	26	4000		
AlcoholL	Y=log (RS/R0)	X=log (ppm)	A	B
	17	50	-0,06122	1,3345
	13	4000		
CH4	Y=log (RS/R0)	X=log (ppm)	A	B
	15	50	-0,11657	1,3741
	9	4000		
LPG	Y=log (RS/R0)	X=log (ppm)	A	B
	9	50	-0,13414	1,1821
	5	4000		
CO	Y=log (RS/R0)	X=log (ppm)	A	B
	1	100	-0,65276	1,3055
	0,09	4000		
H2	Y=log (RS/R0)	X=log (ppm)	A	B
	0,8	100	-2,0588	4,0207
	0,02	600		

AIR

$$\log\left(\frac{R_s}{R_0}\right) = 1,415 \leftrightarrow \frac{R_s}{R_0} = 10^{(1,4149)} = 26$$

CO

$$\log\left(\frac{R_s}{R_0}\right) = -0,6527 * \log(x) + 1,3055$$


$$= A * \log(x) + B$$

As can see, methane has the highest variation slope on MQ-4. It is followed by LPG. We will therefore use this sensor for detecting methane in produced gases.


### 2.3.4 Putting these gases sensors together

In case of gasification, we seek to produce mainly carbon monoxide and hydrogen, plus sometime methane.

The stoichiometric combustion of wood in air containing 21% of oxygen and 79% of nitrogen is the following equation:



When oxygen is not supplied in sufficient quantity, CO is produced in lieu and place of CO<sub>2</sub>. Also, water vapor is engaged in the so-called water-gas shift reaction that produce hydrogen as a reaction between carbon dioxide and water vapor according equation 2 to below:



Consequently, we have mixture of CO, H<sub>2</sub>, CH<sub>4</sub>, CO<sub>2</sub> and N<sub>2</sub> from the gasification of biomass.

Knowing the concentrations of each of these gases thank to MQ sensors will help us monitor the gasification process.

These gases concentration will be calculated with a microcontroller as a computer under the Microchip Integrated Development Environment (IDE) named MPLAB IDE v8.80.

## 3. Results and discussion

### 3.1 Calibration of the MQ gas sensors

Calibration of MQ gases sensors mainly consist in the determination of resistance Rs. For a concentration x given in ppm, we obtain an electrical resistance Rs at the sensor output through the following properties:

Commented [U15]: Reframe the sentence

#### 3.1.1. Mathematical equations for using gas sensors

Through the calibration curves, we know that:

$$\log\left(\frac{R_s}{R_0}\right) = A * \log(x) + B$$

If we note x the gas concentration in ppm, A and B the constants depending on the type of sensor used, the we can deduce:

$$x = 10^{\left(\frac{\log\left(\frac{R_s}{R_0}\right) - B}{A}\right)} \quad \text{or also}$$

$$\frac{R_s}{R_0} = 10^B * x^A \quad \text{or also}$$

$$x = \left(\frac{R_s}{R_0} * 10^{-B}\right)^{\frac{1}{A}}$$

We have summarized the values obtained for A and B in the two Table 4 and Table 5 below.

Table 4 :Parameter A values of the 3 gas sensors

MQ4 (CH4)	MQ7 (CO)	MQ8 (H2)
-0,3072	-0,6527	-1,522

Table 5 : Parameter B values of the 3 gas sensors

MQ4 (CH4)	MQ7 (CO)	MQ8 (H2)
0,921	1,3055	4,5686

Hence the following mathematical functional block in steady state for each sensor:

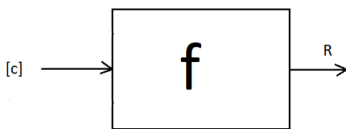


Figure 7 : Functional bloc of the sensors

[C]=x: concentration of the inlet gas.  
R=Rs: output resistance.

f: the mathematical steady-state input-output correlation function.

### 3.1.2. Measurement range

The Table 6, Table 7 and Table 8 above represent the measurement ranges of the sensors.

Table 6 : H2 : MQ8

X= [C] (ppm)	100	10000
RS (kΩ)	10	60

Table 7 : CO : MQ-7

X= [C] (ppm)	10	10000
RS (kΩ)	2	20

Table 8 : CH4 : MQ-4

X= [C] (ppm)	100	10000
RS (kΩ)	10	60

### 3.1.3 Intrinsic sensitivity of the sensors

Intrinsic sensitivity of sensors for a variation of the output  $\Delta R$  of the output, we can estimate the sensitivity through the input variation  $\Delta x$ .

It is equal to:

```
void gaz_processing (int8 canal_in)
// gas concentrartion measurement fonction

{
float yy, xx,m, b0;
int16 reste;
// computing of correction coefficients
// according to humidity
k_rh_mq4= (val_humidity /-322.6)+ 1.10;
k_rh_mq7= (val_humidity/-370.4)+ 1.09;
if (canal_in==0)
{
k_r=1.1560; //k_r= r1_mq7/r0_mq7;
//k_g=0.889024;

k_t_mq7=0.9408; //à 34 degré celcius
k_g= k_t_mq7 * k_rh_mq7;
m=1.0/a_mq7;
b0=20.2069143 ;//b0= pow(10,b_mq7);
vs=vs_mq7;
}

if (canal_in==1)
{
k_r=1.1599; //k_r= r1_mq4/r0_mq4;
//k_g=0.887494;

k_t_mq4=0.9578;
k_g= k_t_mq4 * k_rh_mq4;
m=-3.25520833;//m=1.0/a_mq4;
b0=8.33681185 ;//b0= pow(10,b_mq7);
vs=vs_mq4;
}
}
```

$$\frac{\partial x}{\partial R_s} = \frac{1}{A} * \left(\frac{10^{-B}}{R_0}\right) * \left(\frac{R_s}{R_0} * 10^{-B}\right)^{\left(\frac{1-A}{A}\right)}$$

### 3.1.4 Implementation in MPLAB IDE

MPLAB IDE is written in C language. Equation from different sensors were derived for each sensor and we obtained results summarized below.




Figure 8 : Microchip MPLAB IDE logo

Commented [U18]: Plate (image) after it is equal to : should be properly check again for consistencies and caption be given to it.

Commented [U19]: Check this sentence please

Commented [U16]: Find a way of placing these results(Table4 and 5) in your abstract. in discussing results related literature should be used to support findings of the current research.

Commented [U17]: Tables 6,7 and 8 captions should be reframe to reflect the content of the tables

```

void main(void) // main fonction
{
  init_uc(); //microcontrôleur initialisati

  while(1) // loop
  {

    // mesurment of gas conetration
    if(gaz_process==1)
    {
      gaz_process=0;
      acquisition ();
      integration(0);
      gaz_processing (0);
      integration(1);
      gaz_processing (1);
    }

    // measurement of humidity
    if(fin_hum)
    {
      fin_hum=0;
      humidity_processing ();
    }
  }
}

```

Figure 9 : The main bloc of our program

As we can see on Figure 9 above, the main program is subdivided in six routines that do a given work. The most important of these is “gaz\_processing ( )” that calculate the different concentrations of the gases as illustrated on Figure 10 below:

https://www.timeanddate.com/weather/burkina-faso/koudougou/historic

News World Clock Time Zones Calendar Weather Sun, Moon

### High & Low Weather Summary for septembre 2023

	Temperature	Humidity	Pressure
<b>High</b>	36 °C (11 sep, 14 h 00)	100% (1 sep, 02 h 00)	1016 mbar (1 sep, 02 h 00)
<b>Low</b>	22 °C (2 sep, 19 h 00)	47% (30 sep, 13 h 00)	1007 mbar (12 sep, 17 h 00)
<b>Average</b>	29 °C	78%	1012 mbar

\* Reported 1 sep 02 h 00 — 30 sep 23 h 00, Koudougou. Weather by CustomWeather, © 2024

Note: Actual official high and low records may vary slightly from our data, if they occurred in-between our weather recording intervals... More about our weather records

Figure 10 : The gases concentrations calculation function of the program

### 3.2 Electronic prototype

From the electronic diagrams, we were able to create some prototype power supply and conditioning boards ( and ). The measurement cards are made with Pic-kit cards from Microchip and Arduino uno.

The measurement system was fabricated with prototyping board and assembled together. The power supply board provides 5V, +8V and -8V voltages to the sensors and measurement amplifiers. as seen below:

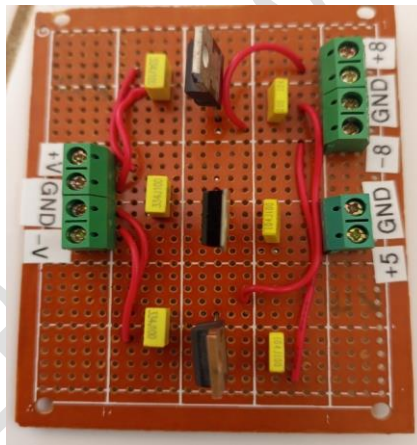


Figure 11 : Main power module

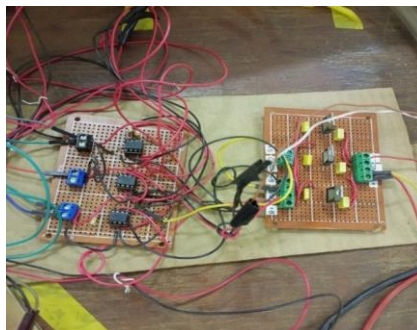


Figure 12 : Treatment and power supply boards

### 3.4 Tests results

On September 23, 2023, gasification measurement tests were carried out and obtained CH4 concentration values = 310 ppm; CH4=10ppm; RH= 72%. Figure 13 represents a local display on an LCD screen

of the gasification parameters obtained during the test.

These values were lesser than those we go from previous experiments in nearly similar experimental conditions: waste weigh, weather, etc.



Figure 13 : Test results on LCD display

These measurement results show low production of combustible gas. The air-dried wood used did not seem to have any problems and it had not rained in the 2 days preceding our handling. At that time, the oxygen concentration measurement module was not yet ready and we did not understand the reason for the failure of our manipulation. On November 1, 2023 at 5 p.m., we then took measurements of the humidity level of the ambient air. There we found 51%. On January 10, 2024, the indicated humidity level was 8%. We then looked for the causes of these differences in values and consulted the history of the weather in Koudougou. So, for September 23, 2023, the following screenshot shows

## 5. REFERENCES

1 Joan Nyika, Adeolu Adesoji Adediran, Adeniyi Olayanju, Olanrewaju Seun Adesina and Francis Odikpo Edoziuno, The Potential of Biomass in Africa and the Debate on its Carbon Neutrality,

that the weather forecast indicated between 65 and 75% air humidity:

Figure 14 : Weather in Koudougou during September 2023

Conclusion therefore made that our gas measurement system is working as intended.

## 4. Conclusion

Through this study, the operation of gas concentration sensors made by Hanwey Corp was highlighted. The test body of these sensors is a layer of tin dioxide ( $\text{SnO}_2$ ) whose resistivity is sensitive to contact gases and varies according to their concentration. The electrical model of these sensors is a resistance whose measurand is the concentration of the gas in contact. Thus, we were able to find the first physico-mathematical model of the  $\text{CO}$ ,  $\text{H}_2$ ,  $\text{CH}_4$  gas sensors of the experimental gasifier. An electronic prototype was built and was used to measure  $\text{CO}$  and  $\text{CH}_4$  concentrations together with relative humidity successfully. The same method was applicable for  $\text{H}_2$ . However, these sensors were very sensitive to the temperature and humidity of the gases measured. These auxiliary parameters were the subject of a study which make it possible to find the real physical and mathematical model allowing judicious exploitation of these sensors.

Biotechnological Applications of Biomass, DOI: 10.5772/intechopen.93615, 2020

2 Sustainable Energy for All, [Burkina Faso]: Rapid assessment and gap analysis, pp. 1-2, [https://www.seforall.org/sites/default/files/Burkina\\_Faso\\_RAGA\\_FR\\_Released.pdf](https://www.seforall.org/sites/default/files/Burkina_Faso_RAGA_FR_Released.pdf), Accessed 26 septembre 2023. French.

Commented [U20]: Where is the figure ?

Commented [U21]: Try to make your conclusion in term of quantity.

Commented [U22]: Make sure you adhere to your publisher template in listing of your references.

---

3 Nzihou Jean Fidele, Hamidou Salou, Imbga Kossi, Segda Bila Gerard, Ouattara Frederic, Tientore Hamadou, Electrical Power Generation from Heat Recovered at the throat of a Downdraft Biomass Gasifier, American Journal of Science, Engineering and Technology, 2023; 8(3) : 133-140, <http://www.sciencepublishinggroup.com/j/ajset>  
doi: 10.11648/j.ajset.20230803.12, ISSN: 2578-8345 (Print); ISSN: 2578-8353 (Online)

4 Nzihou Jean Fidele, Hamidou Salou, Segda Bila Gerard, Ouattara Frederic and Compaore Hamidou, Effects of a Cyclone Dimensions on Quality of Syngas Produced with a Wood-fired Biomass Gasifier, Journal of Energy Research and Reviews, Article number JENRR.107030, ISSN: 2581-8368, Volume 15, Issue 3, Page 1-14, 2023

5 Yulin Kong, Yuxiu Li, Xiuxiu Cui, Linfeng Su, Dian Ma, Tingrun Lai, Lijia Yao, Xuechun Xiao, Yude Wang, SnO<sub>2</sub> nanostructured materials used as gas sensors for the detection of hazardous and flammable gases: A review, Nano Materials Science, Volume 4, Issue 4, 2022, Pages 339-350, ISSN 2589-9651, <https://doi.org/10.1016/j.nanoms.2021.05.006>, 2022

6 I Kadek NuaryTrisnawan, Agung Nugroho Jati, Novera Istiqomah, Isro Wasisto, Detection of Gas Leaks Using The MQ-2 Gas Sensor on the Autonomous Mobile Sensor,

7 Nisal Kobbekaduwa, Pahan Oruthota and W.R. de Mel, Calibration and Implementation of Heat Cycle Requirement of MQ-7 Semiconductor Sensor for Detection of Carbon Monoxide Concentrations, Advances in Technology. 2021, 1(2), 377-392

8 Sohibun, I Daruwati, R G Hatika and D Mardiansyah, MQ-2 Gas Sensor using

Micro Controller Arduino Uno for LPG Leakage with Short Message Service as a Media Information, URICSE 2021, Journal of Physics: Conference Series, (2021) 012068 IOP Publishing, doi:10.1088/1742-6596/2049/1/012068

8 Abubakar Yakub Nasir<sup>1</sup>, U. I. Bature<sup>2</sup>, N. M. Tahir<sup>3</sup>, A. Y. Babawuro<sup>4</sup>, Adoyi Boniface<sup>5</sup> A. M. Hassan, Arduino based gas leakage control and temperature monitoring system, International Journal of Informatics and Communication Technology (IJ-ICT), Vol.9, No.3, December 2020, pp. 171-178, ISSN : 2252-8776, DOI : 10.11591/ijict.v9i3.pp171-178  
Journal homepage: <http://ijict.iaescore.com>, 2020

10 Huan Hui Yan, Yusnita Rahayu, Design and Development of Gas Leakage Monitoring System using Arduino and ZigBee, Proceeding of International Conference on Electrical Engineering, Computer Science and Informatics (EECSI 2014), Yogyakarta, Indonesia, 20-21 August 2014

11 L Dewi and Y Somantri, Wireless sensor network on lpg gas leak detection and automatic gas regulator system using Arduino, IOP Conf. Serie: Material Sciences Engineering, 384 012064, 2018

12 Laghrib Souad, Synthesis of Thin Films of: SnO<sub>2</sub>, SnO<sub>2</sub>: In by Two Physical and Chemical Processes and Study of Their Characterization, PhD Thesis, Ferhat Abbas University, Algeria, 139 pages, 2018. French.

13 J. Jacquemin. Optical PROPERTIES OF Intrinsic SnO<sub>2</sub> AND  $\beta$ -PbO<sub>2</sub> neighborhood of the gap. Journal de Physique Colloques, 1974, 35 (C3), pp. C3-255-C3-260. 10.1051/jphyscol:1974337. jpa-00215585

14 Laghrib Souad, Hania Amardjia-Adnani, Dahir Abdi, Jean-Marc Pelletier, Development and study of thin layers of

---

SnO<sub>2</sub> obtained by evaporation under vacuum and annealed under oxygen, Revue des Energies Renouvelables Volume 10 N°3 (2007) 357–366, 2007. French.

15 Priyanka Kakoty and Manabendra Bhuyan, SnO<sub>2</sub> based gas sensors: Why it is so popular?

UNDER PEER REVIEW